

## Auto-Fill Adherence Packaging




### SEALING INSTRUCTIONS FOR SYNMED<sup>®</sup> AUTOMATED FILLING

Ensuring the printed/front side of the panel is facing down, place the grid panels over the card positions in the SynMed<sup>®</sup> tray (1).


Place the blisters through each grid panel and into the tray (2).

When all of the panels and blisters have been placed, insert the tray into the SynMed machine and follow SynMed instructions to operate the machine (3). When the filling process is complete, remove the tray as instructed to begin the sealing process. Please note each step below will be repeated across all 12 cards in the tray.

Once the loaded medications have been verified for accuracy, locate the pre-separated adhesive panel (4a) and remove the liner (4b).

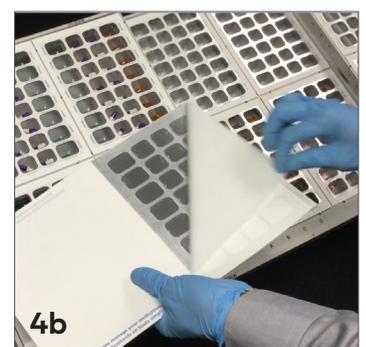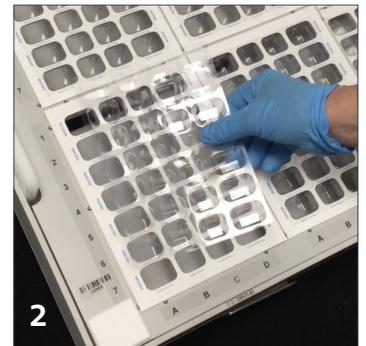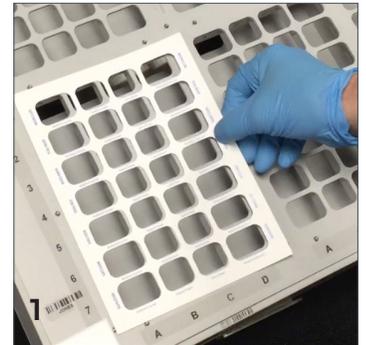



With the adhesive side facing down, orient the adhesive panel over the blister and grid panel on the tray (5a). Align the adhesive panel with the alignment pins on the SynMed tray to ensure the panel is positioned accurately (5b).

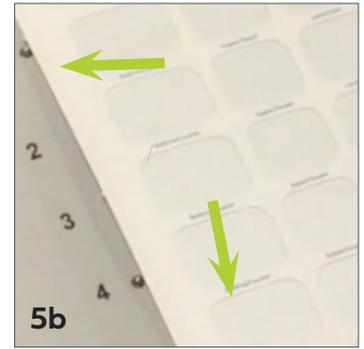


Apply pressure to the panel to engage the adhesive (6a). Avoiding the pins, use a 4" roller to apply pressure in a vertical and horizontal motion. Roll multiple times and ensure the roller reaches all edges of the card to create a tight seal (6b).



Turn the card over. Then, peel the medication summary label (7a) and affix to the inside cover (7b). The pharmacist must verify the contents.

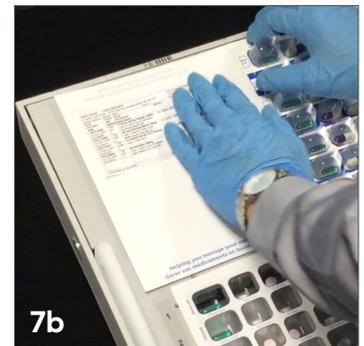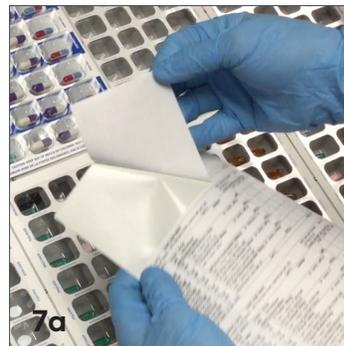

The Auto-Fill is now ready to dispense (8).

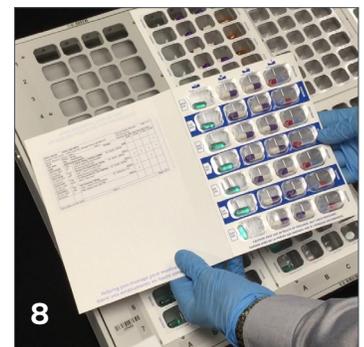

Before dispensing, the pharmacist should instruct the patient on the proper use of the Auto-Fill. To access the contents of a blister, the patient can turn over the package and puncture the blister backing, then peel back the label and remove medication. The pharmacist must also advise the patient that the Auto-Fill is not child-resistant. Keep out of the sight and reach of children and store in a cool, dry place, away from direct sunlight.